



Improved Late Gadolinium Enhancement Imaging of Left Ventricle with Isotropic Spatial Resolution

Citation

Akcakaya, Mehmet, Hussein Rayatzadeh, Susie Hong, Thomas H. Hauser, Raymond H. Chan, Tamer A. Basha, Kraig V. Kissinger, Beth Goddu, Warren J. Manning, and Reza Nezafat. 2012. Improved late gadolinium enhancement imaging of left ventricle with isotropic spatial resolution. *Journal of Cardiovascular Magnetic Resonance* 14(Suppl 1): 022.

Published Version

doi:10.1186/1532-429X-14-S1-022

Permanent link

<http://nrs.harvard.edu/urn-3:HUL.InstRepos:10060085>

Terms of Use

This article was downloaded from Harvard University's DASH repository, and is made available under the terms and conditions applicable to Other Posted Material, as set forth at <http://nrs.harvard.edu/urn-3:HUL.InstRepos:dash.current.terms-of-use#LAA>

Share Your Story

The Harvard community has made this article openly available.
Please share how this access benefits you. [Submit a story](#).

[Accessibility](#)



ORAL PRESENTATION

Open Access

Improved late gadolinium enhancement imaging of left ventricle with isotropic spatial resolution

Mehmet Akcakaya^{1*}, Hussein Rayatzadeh¹, Susie Hong¹, Thomas H Hauser¹, Raymond H Chan¹, Tamer A Basha¹, Kraig V Kissinger¹, Beth Goddu¹, Warren J Manning^{1,2}, Reza Nezafat¹

From 15th Annual SCMR Scientific Sessions
Orlando, FL, USA. 2-5 February 2012

Background

Recent studies have shown the prognostic value of the infarct border zone of late gadolinium enhancement (LGE) images in patients with myocardial infarction [1]. This border zone has also been associated with ventricular arrhythmia [2,3]. The accuracy of the characterization of this area depends on spatial resolution of the imaging. 3D LGE allows improved spatial resolution, especially in through-plane direction. However imaging with an isotropic spatial resolution necessitates very long scan time. In this study, we sought to investigate if compressed-sensing (CS) based image acceleration method [4] allows LGE imaging with isotropic spatial resolution.

Methods

A prospective random under-sampling LGE acquisition was implemented on 1.5T Philips scanner. A free-breathing ECG-triggered inversion-recovery GRE sequence with navigator-gating was used for all acquisitions on 18 patients (5 females, 52.8±16.3 years) 10 to 20 minutes after bolus infusion of contrast agent. Each subject were imaged using two LGE sequence in random order: a) a 3-fold-accelerated LGE scan with isotropic spatial resolution of 1.2-to-1.7 mm³, b) LGE scan with non-isotropic resolution of 1.7×1.7×4.0mm³ were performed with imaging parameters of TR/TE/α=5.2/2.6ms/25°, FOV=320×320×100mm³. Random undersampling was implemented as described in [5], where the central k-space (45×35 in ky-kz) was fully-sampled. Acquisition times were 3 mins assuming 100% scan efficiency at 70 bpm for both scans. The images from the

accelerated scans were reconstructed using an advanced CS-technique, called LOST [4].

Results

Figure 1 shows LGE images from a patient with hypertrophic cardiomyopathy acquired using two different approaches. An improved isotropic spatial resolution allows better characterization of the scar morphology. Figure 2 shows another example in a patient undergoing ICD implantation as a primary prevention of sudden cardiac death.

Conclusions

Accelerated LGE imaging with isotropic spatial resolution allows improved visualization of scar morphology. Further quantitative measurements of infarct border zones in a larger cohort of patients are needed to better understand the prognostic value of the improved scar imaging.

Funding

NIH R01EB008743-01A2.

Author details

¹Medicine, Beth Israel Deaconess Medical Center, Harvard Medical School, Boston, MA, USA. ²Radiology, Beth Israel Deaconess Medical Center, Harvard Medical School, Boston, MA, USA.

Published: 1 February 2012

References

1. Yan : *Circulation*. 2006.
2. Bello : *JACC*. 2005.
3. Nazarian : *Circulation*. 2005.
4. Akcakaya : *MRM*. 2011.
5. Basha : *ISMRM*. 2011.

¹Medicine, Beth Israel Deaconess Medical Center, Harvard Medical School, Boston, MA, USA

Full list of author information is available at the end of the article

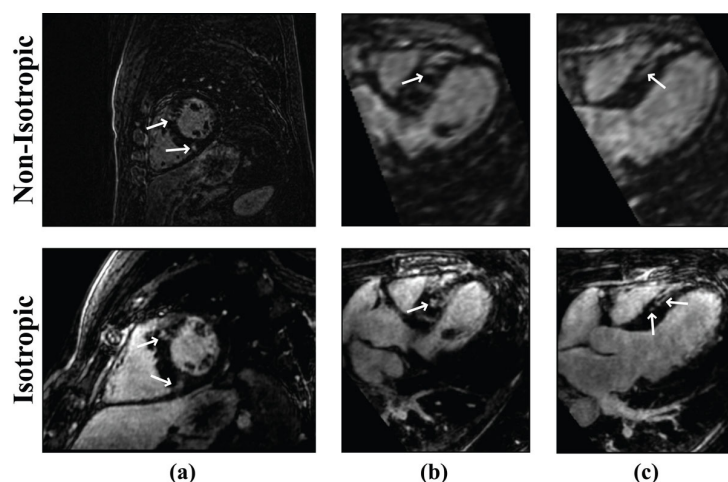


Figure 1 Reformatted LGE images from a patient with HCM, acquired using non-isotropic spatial resolution (top), and isotropic spatial resolution (bottom). An isotropic resolution allows better visualization of scar morphology in images acquired using LOST-accelerated acquisition.

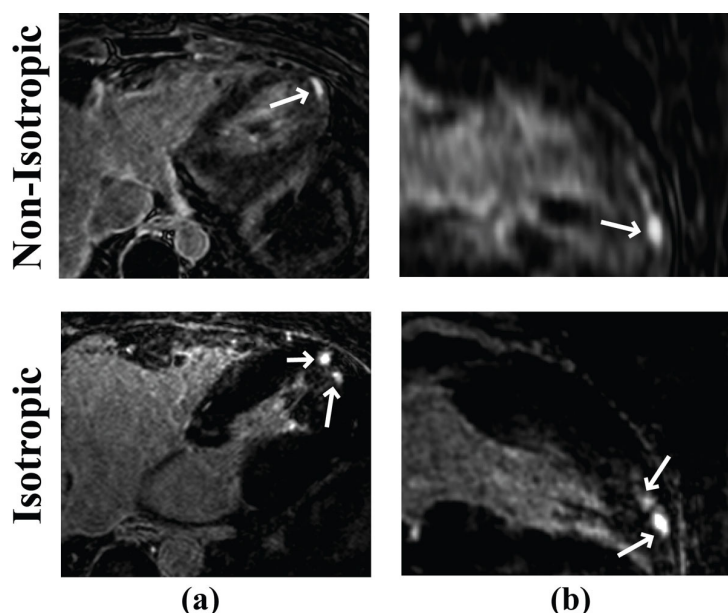


Figure 2 Axial (left) and reformatted long-axis (right) LGE images from a patient. Non-isotropic LGE was acquired with a spatial resolution $1.7 \times 1.7 \times 4.0 \text{ mm}^3$ (top), whereas LOST-reconstructed isotropic resolution images from the accelerated scan had a resolution of $1.2 \times 1.2 \times 1.2 \text{ mm}^3$ (bottom).

doi:10.1186/1532-429X-14-S1-O22

Cite this article as: Akcakaya et al.: Improved late gadolinium enhancement imaging of left ventricle with isotropic spatial resolution. *Journal of Cardiovascular Magnetic Resonance* 2012 **14**(Suppl 1):O22.

Submit your next manuscript to BioMed Central and take full advantage of:

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

